



DASNY

BID NO.:621	PROJECT NAME & LOCATION	New York Psychiatric Institute 1051 Riverside Dr. New York, NY 10032
Description: Furnish & Deliver Laboratory Steam Sterilizer		
Bid Open Location: DASNY 515 Broadway, Albany, NY 12207		
Bid Open Date: December 6, 2018		
Bid Open Time: 2:30 PM		Contact: Peter Bujanow (518) 257-3080

NOTICE TO BIDDERS

MAIL BIDS EARLY

Sealed bids will be received by DASNY at the above address for the items listed in the attached Bid Breakdown and Schedule. When submitting your bid you must:

1. Prepare your bid on the attached Bid Breakdown and Schedule. Return one signed original of the Bid Breakdown and Schedule
2. If your bid deviates from Specifications, explain such deviations or qualifications on your letterhead, setting forth therein such explanations, and attach them to the Bid Breakdown and Schedule.
3. Submission of a bid constitutes full knowledge and acceptance of all provisions of the Notice to Bidders, all information referenced in the Purchasing General Conditions, Supplemental and Detailed Specifications, the Bid Submission and any Supplemental General Requirements contained herein, as well as any addenda issued in relation to the Invitation for Bids.
4. Each bid shall bear on the outside of the envelope the name of the bidder, address, telephone number and designated as a bid for the following:
DASNY Bid No. 621 - Furnish & Deliver Laboratory Steam Sterilizer
Bid Opening Date: December 6, 2018 @ 2:30PM
Return to:
DASNY
Attn: Purchasing Unit
515 Broadway
Albany, NY 12207-2964



Bid No.: 621

When a sealed bid is placed inside another delivery jacket, the bid delivery jacket must be clearly marked on the outside “**BID ENCLOSED**” and “**ATTENTION: PURCHASING UNIT**”. The Dormitory Authority will not be responsible for receipt of bids which do not comply with these instructions.

5. Mail bid responses early in order for them to be received before the time of the bid opening. **Late bids will be automatically rejected.** Individuals submitting bids in person or by private delivery services should allow sufficient time for processing through building security to assure that the bids are received prior to the deadline for submitting bids. All individuals who plan to attend bid openings will be required to present government-issued picture identification to building security officials and obtain a visitor’s pass prior to attending the bid opening.

6. In accordance with State Finance Law § 139-j and 139-k, this solicitation includes and imposes certain restrictions on communications between Dormitory Authority personnel and an Offerer during this procurement process. Designated contact for this solicitation is: Peter Bujanow, Sr. Purchasing Coordinator , at Dormitory Authority – State of New York, 515 Broadway, Albany, NY 12207,(518) 257-3080. Contacts made to other Dormitory Authority Personnel regarding this procurement may disqualify the Offerer and affect future procurements with governmental entities in the State of New York. Please refer to the Authority’s website www.dasny.org for Authority policy and procedures regarding this law, or the NYS office of General Services website www.ogs.ny.gov/BU/PC/ for more information about this law.



NEW YORK
STATE OF
OPPORTUNITY.

DASNY

Bid No.: 621

If you are not submitting a bid it is requested that you complete and return the lower portion of this form

(Please check all that apply and provide comments in the space provided, if necessary)

- We are not Submitting a bid.
- We Request removal of our name from the mailing list.
- Location of the job site.
- Commodity is not carried by our company.
- Scope is too large.

Other/Additional Explanation: _____

NAME OF BIDDER: _____

ADDRESS _____

:
Street City State Zip
Telephone

Signature of Bidder

Official Title



DASNY

CLAUSES PURSUANT TO THE OMNIBUS PROCUREMENT ACT OF 1992

It is the policy of New York State to maximize opportunities for the participation of New York State business enterprises, including minority and woman-owned business enterprises as bidders, subcontractors and suppliers on its procurement contracts.

Information on the availability of New York subcontractors and supplies is available from:

Empire State Development
Small Business Division
30 South Pearl Street, 7th Floor
Albany, NY 12207
Phone: (800) 782-8369

A directory of minority and woman-owned business enterprises is available from:

Empire State Development
Division of Minority and Women Business Development
30 South Pearl Street
Albany, NY 12207
Phone: (518) 292-5250

Online Directory: <https://ny.newnycontracts.com/FrontEnd/VendorSearchPublic.asp>

DASNY maintains a directory of minority and women-owned business enterprises:
<http://www.dasny.org/construc/mwsbereg/index.php>

The contractor acknowledges notice that New York State may seek to obtain offset credits from foreign countries as a result of this contract and agrees to cooperate with the State in these efforts.

DASNY encourages the use of recycled Materials in the manufacturing process. To that end, the recycled product must meet the same codes, specifications and standards the non-recycled materials do, including requirements for cost, installation, aesthetics, availability and maintenance.



The Omnibus Procurement Act of 1992 and § 2879 of the NYS Public Authorities Law require that by signing this bid, contractors certify that whenever the total bid amount is greater than \$1 million:

1. The contractor has made reasonable efforts to encourage the participation of New York State Business Enterprises as suppliers and Subcontractors on this project, and has retained the documentation of these efforts to be provided upon request to the State. If the contractor determines that NYS business enterprises are not available to participate on the contract as subcontractors or suppliers, the contractor shall provide a statement indicating the method by which such determination was made. If the contractor does not intend to use subcontractors, contractor shall provide a statement verifying such;
2. The contractor has complied with the Federal Equal Opportunity Act of 1972 (PL 92-261), as amended;
3. The contractor agrees to make reasonable efforts to provide notification to New York State residents of employment opportunities on this project through listing any such positions with the Job Service Division of the New York State Department of Labor, or providing such notification in such manner as is consistent with existing collective bargaining contracts or agreements. The contractor agrees to document these efforts and to provide said documentation to the State upon request;

DASNY is required by law to notify the NYS Department of Economic Development of any procurement contract for one million dollars or more that is to be awarded to an out-of-state vendor. This notice must be done simultaneous to the notification of award provided to the vendor. A purchase order or contract cannot be issued until fifteen (15) days after such notification is provided.



DASNY

GENERAL SPECIFICATIONS

- (1) The enclosed Purchasing General Conditions are hereby incorporated by reference. Submission of a bid response shall constitute acceptance of such conditions. Any exceptions/clarifications/qualifications to these conditions or other specifications and/or requirements contained herein must be clearly stated in the bid response and, depending upon the nature of such, may be grounds for rejection of your bid.
- (2) Bids must be submitted in the bidder's full legal name, or the bidder's full legal name plus a registered assumed name, if any.
- (3) All NYS bidders are required to be registered to do business with the NYS Department of State or their local County Clerk, whichever is applicable.
- (4) All out-of-state bidders will be required to provide proof of registration to do business in their state. All out-of-state bidders that "do business in New York State" **MUST BE REGISTERED WITH THE NYS DEPARTMENT OF STATE**. Please contact the NYS Department of State at (518) 473-2492. Information is available at the DOS website: www.dos.ny.gov
- (5) DASNY is required by law to notify the Empire State Development of any procurement contract for one million dollars or more that is to be awarded to an out-of-state vendor. This notice must be done simultaneous to the notification of award provided to the vendor. A purchase order or contract cannot be issued until fifteen (15) days after such notification is provided.
- (6) Empire State Development is required by law to identify states and other jurisdictions that impose preferences or other penalties against New York bidders. DASNY is precluded from soliciting bids or entering into procurement contracts with companies that have their principal place of business located in one of the listed jurisdictions, unless the procurement is for a product that is substantially manufactured in New York State or the services are to be performed in New York State. Currently, this list of jurisdictions includes the states of Alaska, Hawaii, Louisiana, South Carolina, West Virginia and Wyoming.
- (7) Unless otherwise indicated, any reference to brands or model numbers is intended to establish a standard. Items of all manufacturers will be considered, provided the item is determined to meet or exceed the required specification. DASNY's decision as to whether a substitute item meets specification will be final. Your attention is directed to Article II-7, Page 5 of the General Conditions. In order to evaluate substitute items, detailed specifications must be submitted for any product that is other than the one(s) specified in the bid.



NEW YORK
STATE OF
OPPORTUNITY.

DASNY

GENERAL SPECIFICATIONS CONTINUED

- (8) Unless otherwise noted, guarantee on all items is to be one year as detailed in Article XVI of the General Conditions
- (9) All upholstered furniture and drapery panels and lining must meet strict flammability requirements. Standards applicable to this bid, if any, will be delineated in the Detailed Specifications.
- (10) LABOR/TRADES - Any labor, materials or means whose employment, or utilization during the course of this contract, shall not in any way cause or result in strike, work stoppages, delays, suspension of work; or similar troubles by workers employed by this contractor or his subcontractors, or by any of the trades working in or about the buildings and premises where work is being performed. Any violation by the contractor of this requirement may in the sole judgment of DASNY be considered as proper and sufficient cause for declaring the contractor to be in default, and for the owner to take action against him as set forth in the Purchasing General Conditions, Article VIII, "Termination", or such other action as DASNY may deem proper.
- (11) Bid results are available on the DASNY website (www.DASNY.org). Bid results will not be given over the phone.
- (12) If you are a NYS Certified Minority or Women Owned Business, please include a copy of your certification with the bid.



DASNY

ANDREW M. CUOMO
Governor

ALFONSO L. CARNEY, JR.
Chair

GERRARD P. BUSHELL, Ph.D.
President & CEO

SUPPLEMENTAL SPECIFICATIONS

The following items are attached for informational purposes. Referenced documents need not be returned with the proposal. These documents are only applicable to the successful bidder and the ensuing procurement contract. Documents are only applicable to the successful bidder and the ensuing procurement contract. Documents applicable to the procurement that will result from this Invitation for Bids are designated by a check box (☒). Unless otherwise indicated, the referenced documents are located at the end of this Invitation for Bids.

- Purchasing General Conditions** – The DASNY Purchasing General Conditions contains terms and conditions of purchases made by DASNY. It is recommended that this document be reviewed fully.
- M/WBE Utilization Plan and Request for Waiver** - Minority and Women-Owned Business Enterprise (M/WBE) goals for this project are ___% and ___%, respectively. The successful bidder shall be required to complete a Utilization Plan or Request for Waiver, to be approved by DASNY's Opportunity Programs Group. Reference Purchasing General Conditions, Article XIX, Affirmative Action for Contracts Mr. Michael Clay, DASNY Opportunity Programs Group at (518) 257-3464, is available to assist all bidders in attaining these goals. *Reference the enclosed "Good Faith Efforts Guidelines".*
- Supplemental General Requirements** – Attached (if applicable) are the Supplemental General Requirements (SGRs) which provide important logistical information and additional conditions which govern this procurement. Please read these SGRs carefully.
- Form of DASNY Contract** – The procurement resulting from the Invitation for Bids will be executed through a DASNY purchase order and a related contract. The contract executed with the successful bidder will be in the same substantial form as the attached "Form of Contract". Note that this Invitation for Bids and any response to such will be annexed as binding terms of the purchase agreement.
- Certificate of Insurance** (*sample enclosed*) – The successful bidder will be required to provide a Certificate of Insurance pursuant to Article XIV of the enclosed Purchasing General Conditions. The certificate shall name DASNY and other designated parties as additional insureds.

CORPORATE HEADQUARTERS
515 Broadway
Albany, NY 12207-2964

T 518-257-3000
F 518-257-3100

NEW YORK CITY OFFICE
One Penn Plaza, 52nd Floor
New York, NY 10119-0098

T 212-273-5000
F 212-273-5121

BUFFALO OFFICE
539 Franklin Street
Buffalo, NY 14202-1109

T 716-884-9780
F 716-884-9787

DORMITORY AUTHORITY STATE OF NEW YORK

**WE FINANCE, BUILD AND
DELIVER.**

www.dasny.org



DASNY

ANDREW M. CUOMO
Governor

ALFONSO L. CARNEY, JR.
Chair

GERRARD P. BUSHELL, Ph.D.
President & CEO

SUPPLEMENTAL SPECIFICATIONS CONTINUED

- Worker's Compensation / Disability Insurance** – The successful proposer will be required to provide specific documentation with respect to Worker's Compensation and Disability Insurance pursuant to Article XIV of the enclosed Purchasing General Conditions. Requirements are detailed in the enclosed "Workers' Compensation and Disability Benefits Requirements" document.

- Prevailing Wage Schedule** – NYS Labor Law requires all wages paid by contractors and subcontractors on public work projects be paid at the prevailing wage rates. Enclosed is the current rate schedule for the appropriate county. Contractors and Subcontractors are responsible for obtaining current rates throughout the course of the project. The NYS Department of Labor (NYS DOL) updates these rates on July 1st of each year. Current rates can be obtained on the NYS DOL website (www.labor.state.ny.us) or by fax at (518) 485-1870. Note that an executed Contractor and Subcontractor Certification and certified payrolls, which include the hours and days worked by each workman, laborer or mechanic, the occupation at which he worked, the hourly wage rate paid and the supplements paid or provided, must be submitted with each and every payment requisition. **DASNY will not process an invoice without this information.** Forms are available on the DASNY website:
<http://www.dasny.org/construc/forms2/vendors.php>

- Labor and Material Payment Bond** – The successful bidder must be prepared to provide surety bonds prior to award in accordance with Article XIV of the DASNY Purchasing General Conditions. The costs of these bonds are to be separately stated in the total bid price as indicated on the Bid Breakdown and Schedule.

- Performance Bond** – The Successful bidder must be prepared to provide surety bonds prior to award in accordance with Article XIV of DASNY Purchasing General Conditions. The costs of these bonds are to be separately stated in the total bid price as indicated on the Bid Breakdown and Schedule.

- Standard Vendor Responsibility Questionnaire (SVRQ)** – The successful proposer, in accordance with Article XXII of DASNY Purchasing General Conditions, will be required to complete the enclosed SVRQ. The award of a contract will be subject to a review of the information contained in these forms.

CORPORATE HEADQUARTERS
515 Broadway
Albany, NY 12207-2964

T 518-257-3000
F 518-257-3100

NEW YORK CITY OFFICE
One Penn Plaza, 52nd Floor
New York, NY 10119-0098

T 212-273-5000
F 212-273-5121

BUFFALO OFFICE
539 Franklin Street
Buffalo, NY 14202-1109

T 716-884-9780
F 716-884-9787

DORMITORY AUTHORITY STATE OF NEW YORK

**WE FINANCE, BUILD AND
DELIVER.**

www.dasny.org

SUPPLEMENTAL GENERAL REQUIREMENTS

DASNY IFB # 621

1. SPECIAL SITE CONDITIONS

The successful bidder shall strictly adhere to all site security and safety requirements administered by the Federal Government, the State of New York State, NYS Department of Mental Health, New York Psychiatric Institute and the Dormitory Authority - State of New York.

CORPORATE HEADQUARTERS

515 Broadway
Albany, New York 12207-2964

T 518-257-3000
F 518-257-3100

NEW YORK OFFICE

One Penn Plaza, 52nd Floor
New York, New York 10119-0098

T 212-273-5000
F 212-273-5121

BUFFALO OFFICE

539 Franklin Street
Buffalo, New York 14202-1109

T 716-884-9780
F 716-884-9787

DETAILED SPECIFICATIONS & DRAWINGS

DASNY

INVITATION FOR BIDS # 621

The following page(s) include Detailed Specifications and/or Drawings for the goods and/or services to be procured.

FURNISH, DELIVER, MOVE TO LOCATION, AND MAKE READY FOR USE **LABORATORY STEAM STERILIZER**

- ❖ Furnish, Deliver, Move to Location and Make Ready for Use, Laboratory Steam Sterilizer as manufactured by Consolidated Sterilizer Systems, Model Number PT-SR-24F:24" x 36" x 72" Chamber Pass-Thru Sterilizer, or equal, including various selected options and features as indicated.

Model PT-SR-24F: 24" x 36" x 72" Chamber Pass-Through Sterilizer with the following features:

Selected Options:

- X1 Controls: 7" Color Touchscreen, up to 50 programmable cycles
- Password Protection (up to 50 users & passwords) and Lockable Cycle Parameters
- Impact Printer
- Cloud-based monitoring & data collection (1-year subscription) for X1
- Door Interlock System with Dual Control Option (includes 7" secondary screen)
- Controls: 110 volts, 60 Hz (standard) - Controls Monitoring (TBD at time of order)
- Nickel Clad Chamber with Carbon Steel Jacket
- House Steam
- Premium Hi-Vacuum System with Liquid Ring Pump - Vacuum Pump Voltage & Phase (TBD at time of order)
- Brass, Bronze and Copper Piping
- Door Hinge Side (TBD at time of order)
- WaterEco Vacuum Plus with Automatic Wastewater Cooling
- Automatic Jacket Blowdown for Liquids Cycle
- Stationary Bottom Shelf & Stationary Upper Shelf with one (1) Angle Shelf Support
- Two (2) LoADING Carts, Two (2) Transfer Carriages, Chamber Tracks
- Ethernet Port



Standard Features:

- Cloud-based Monitoring & Data Collection Systems
- Double Door Configuration
- ASME (American Society of Mechanical Engineers) U-1 Code Stamping
- ½" Thermocouple Port
- UL, Cul Listed
- Hinged, Fully Opening, Manual Door
- Starter Kit including C3 cleaner and scrubbing pads, a pair of autoclave gloves, printer paper and private ribbon (if applicable), and electronic manuals

Installation:

- Includes receiving sterilizer, uncrating, installing the doors, setting into place, leveling, final assembly, final utility connections, start-up, and user training.


Manufacturer Specifications:

- "Consolidated Sterilizers General Specifications: Medium Lab Series Steam Sterilizers, thirteen (13) pages numbered 1 through thirteen"


Manufacturer Drawings:

- "Title: Medium Steam Sterilizer Pass-Thru Cut Sheet ADV PB/PRO/PLUS, Drawing No. 91119, Rev 3, Sheet 1 of 2"
- "Title: Medium Steam Sterilizer Pass-Thru Cut Sheet ADV PB/PRO/PLUS, Drawing No. 91119, Rev 3, Sheet 2 of 2"


END.

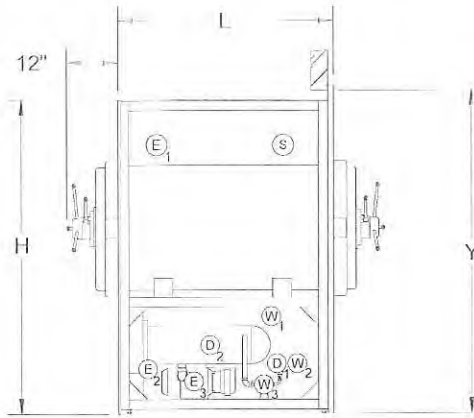


SIDE VIEW

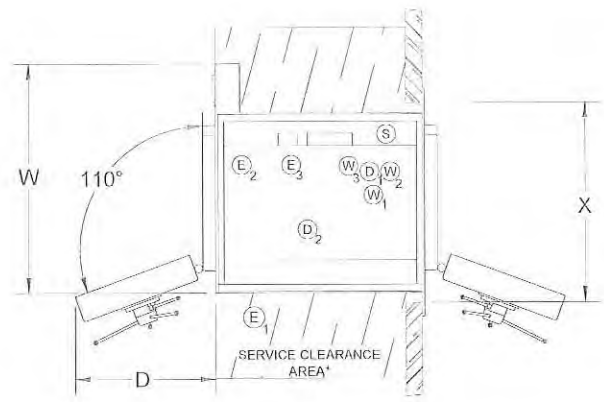

TOP VIEW

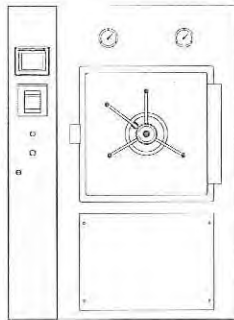

FRONT VIEW
(OPERATING END)

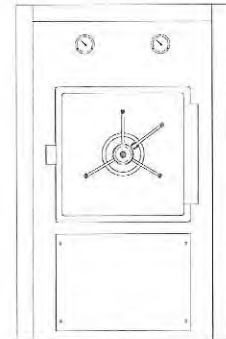

FRONT VIEW
(NON-OPERATING END)

Ⓔ Electrical Ⓓ Drain ⒲ Water Ⓔ Steam

* Recommended service clearance is 18-24" both sides and back

Notes

- Operating end right side control housing, left side door hinge shown. Non-operating end shown with left side optional remote-mounted controller and right side door hinge. Standard control location is opposite hinge. Opposite mounting is available upon request.
- CAD Blocks are available for insertion into plan drawings.
- The control housing is shipped detached from the sterilizer to allow passing through doorways, reducing overall pre-installation width by 10 3/8". When the sterilizer is installed, the control housing and electrical connections are easily attached.
- Standard plumbing and utility access is primarily located on the same side as the door hinge. If location of plumbing is important to your installation contact Consolidated to arrange a solution.

Table 1: Sterilizer Unit Dimensions

Model	PT-SR-24C	PT-SR-24D	PT-SR-24E	PT-SR-24F	PT-SR-26B	PT-SR-28B
Chamber Dimensions (w x h x f-b)	24" x 36" x 36" 61 x 91.4 x 91.4 cm	24" x 36" x 48" 61 x 91.4 x 122 cm	24" x 36" x 60" 61 x 91.4 x 152.4 cm	24" x 36" x 72" 61 x 91.4 x 183 cm	26" x 26" x 49" 66 x 66 x 124.5 cm	28" x 28" x 48" 71 x 71 x 122 cm
Volume	18 cu. ft 510 liters	24 cu. ft 680 liters	30 cu. ft 850 liters	36 cu. ft 1019 liters	19.2 cu. ft 544 liters	21.8 cu. ft 617 liters
Overall Width (W)	48.375" 122.9 cm	48.375" 122.9 cm	48.375" 122.9 cm	48.375" 122.9 cm	48.375" 122.9 cm	51" 129.5 cm
Overall Height (H)	71" 180.3 cm	70.25" 178.4 cm	70.25" 178.4 cm	70.25" 178.4 cm	71" 180.3 cm	71" 180.3 cm
Overall Length (L)	42.5" 108 cm	54.5" 138.4 cm	66.5" 169 cm	78.5" 199.4 cm	49" 124.5 cm	54.5" 138.4 cm
Wall Opening Width (X)	40" 101.6 cm	40" 101.6 cm	40" 101.6 cm	40" 101.6 cm	40" 101.6 cm	43" 109.2 cm
Wall Opening Height (Y)	72" 182.9 cm	71.25" 181 cm	71.25" 181 cm	71.25" 181 cm	72" 182.9 cm	72" 182.9 cm
Door Swing (D)	31.5" 80 cm	31.5" 80 cm	31.5" 80 cm	31.5" 80 cm	35.5" 90.2 cm	37.5" 95.3 cm

1 Additional options may require a larger footprint.
2 Alternative controller mounting options are available at no charge for installations into smaller wall openings. Contact Consolidated or your Consolidated Sales Representative to arrange a solution.

NAME	DATE	CONSOLIDATED STERILIZER SYSTEMS 76 ASHFORD ST, BOSTON MA 02134
DRAWN: S MECHLER	12/20/08	
UPDATED: S MECHLER	10/01/07	
ENG APPR:		
MFG APPR:		
QA		TITLE:
COMMENTS		MEDIUM STEAM STERILIZER PASS-THRU CUT SHEET ADV PB/PRO/PLUS
PROPRIETARY AND CONFIDENTIAL THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF CONSOLIDATED STERILIZER SYSTEMS ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF CONSOLIDATED STERILIZER SYSTEMS IS PROHIBITED.		SIZE DWG. NO. REV A 91119 3 SCALE: N/A WEIGHT: -- SHEET 1 OF 2

Table 2: Power and Steam Usage³

Power and Steam Usage			Electrically Heated					Steam Heated		
Model	Chamber Dimensions (w x h x f-b)	Air Removal Method	Generator Size (kw)	Generator Current (amps) ⁴				Steam Consumption		
				208V	240V	380V	480V	Peak (lb/hr)	Per Cycle (lb/cycle)	Idle (lb/hr)
PT-SR-24C	24" x 36" x 36" 61 x 91.4 x 91.4 cm	Gravity	30	83	72	46	36	180	40	9
		Vacuum	45	125	108	68	54	180	65	9
PT-SR-24D	24" x 36" x 48" 61 x 91.4 x 122 cm	Gravity	30	83	72	46	36	180	45	10
		Vacuum	45	125	108	68	54	180	75	10
PT-SR-24E	24" x 36" x 60" 61 x 91.4 x 152.4 cm	Gravity	60	167	144	91	72	180	50	11
		Vacuum	80-100	222-278	192-240	122-152	96-120	180	105	11
PT-SR-24F	24" x 36" x 72" 61 x 91.4 x 183 cm	Gravity	80	222	198	122	96	180	55	11
		Vacuum	100-120	278-333	240-289	152-182	120-144	180	125	11
PT-SR-26B	26" x 26" x 49" 66 x 66 x 124.5 cm	Gravity	30	83	72	46	36	180	40	9
		Vacuum	45	125	108	68	54	180	70	9
PT-SR-28B	28" x 28" x 48" 71 x 71 x 122 cm	Gravity	30	83	72	46	36	180	40	9
		Vacuum	45	125	108	68	54	180	70	9

3 Assuming 30 Minute sterilizing time at 250°F (121° C) and 20 minute drying time

4 Current drawn by a three phase generator. Local codes and regulations may affect breaker size.

Table 3: Nominal Water Quality Requirements

Characteristic	Carbon Steel Steam Generators ⁵		General Vacuum Device & Quench	
	Recommended Condition	Maximum Condition	Recommended Condition	Maximum Condition
Temperature [°F (°C)]	As Supplied	140 (60)	40-60 (4-16)	70 (21)
Total Hardness (mg/L)	17	85	10-85	171
Alkalinity (mg/L)	50-180	350	50-180	350
Total Dissolved Solids (mg/L)	50-150	250	50-200	500
pH	7.5-8.5	7.5-9.0	6.8-7.5	6.5-9.0
Total Silica (mg/L)	0.1-1.0	2.5	0.1-1.0	2.5
Resistivity (Ω-cm) ⁶	2,000-6,000	26,000	2,000-26,000	500,000

5 Stainless-steel generators require deionized water with resistivity ≥ 1MΩ-cm.

6 If water supplied is greater than 26,000 Ω-cm contact Consolidated for recommendation.

Typical Utility Requirements

General

- Steam (S): ¾" NPT, 50-80 psi dynamic
- Electrical (E): 110V AC, or 220V AC, single phase, 15 amps - dedicated and isolated
- Waste Water Cooling (W): ½" NPT, 45 psi dynamic minimum
- Drain (D): Open drain to funnel connection in floor, diameter 3" minimum, 2-½" air gap
- Backflow preventer not provided
- SteriNET Connex: Ethernet or Analog Phone line, dedicated, non-extension
- Optional Vacuum Systems (maximum one per unit)
 - Economy Post-Vac (E₃): ½" NPT, 45 psi dynamic minimum.
 - Hi-Vacuum with Water Ejector (W₃): 1¼" NPT, 45 psi dynamic minimum
 - Pump contactor (E₃): 110V/220V, single phase
 - Hi-Vacuum with Vacuum Pump (E₃W₃): ½" NPT, 45 psi dynamic minimum, 208/230/460V, three phase
- Electric Steam Generator Utilities:
 - Power Supply (E₂): Available in 208/240/380/480V, single or three phase
 - Generator Feedwater (W₂): Water that complies with Table 3, ½" NPT, 45 psi dynamic minimum
 - Generator Drain (D₂): ¾" NPT

Table 4: Shipping & Heat Loss Data

Model	Max. Ship Weight	Ship Dimensions (w x h x f-b)	Heat Source Options	Max. Operating Weight ⁷	Peak Heat Loss (BTU/hr at 70°F [21°C])			
					Front of Wall	Back of Wall	Front of Walls	Between Walls
PT-SR-24C	3150 lbs 1432 kg	48" X 78" X 72" 121.9 X 198.1 X 182.9 cm	Steam	3300 lbs	5000	11400	5000	7100
			Electric	3475 lbs	5800	12850	5800	7750
PT-SR-24D	3600 lbs 1637 kg	48" X 78" X 84" 121.9 X 198.1 X 213.4 cm	Steam	3825 lbs	5000	13800	5000	8800
			Electric	4000 lbs	5800	15250	5800	9450
PT-SR-24E	4050 lbs 1841 kg	48" X 78" X 96" 121.9 X 198.1 X 243.8 cm	Steam	4375 lbs ⁸	5000	16500	5000	10500
			Electric	4375 lbs ⁸	5800	17950	5800	11150
PT-SR-24F	4750 lbs 2160 kg	48" X 78" X 108" 121.9 X 198.1 X 274.3 cm	Steam	5175 lbs	5000	19200	5000	12000
			Electric	5175 lbs ⁸	5800	20650	5800	12650
PT-SR-26B	2950 lbs 1338 kg	46" X 77" X 79" 117 X 196 X 201 cm	Steam	3250 lbs	5000	10190	5000	5190
			Electric	3425 lbs	5700	11940	5700	6240
PT-SR-28B	3350 lbs 1523 kg	48" X 76" X 91" 121.9 X 193 X 231.1 cm	Steam	3625 lbs	4800	12600	4800	7950
			Electric	3800 lbs	5600	14050	5600	8600

7 Assuming chamber fully loaded with flasks filled 25% with water.

8 Remote mounted generator.

DATE	9/15/2010	CONSOLIDATED STERILIZER SYSTEMS 76 ASHFORD ST. BOSTON MA 02134 TITLE: MEDIUM STEAM STERILIZER PASS-THRU CUT SHEET ADV PB/PRO/PLUS SIZE DWG. NO. A 91119 REV 3 SCALE: N/A WEIGHT: — SHEET 2 OF 2
DRAWN	M. PETERS	
UPDATED	S. MITCHER 10/20/17	
ENG APPR		
MFG APPR		
DATE		PROPRIETARY AND CONFIDENTIAL THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF CONSOLIDATED STERILIZER SYSTEMS. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF CONSOLIDATED STERILIZER SYSTEMS IS PROHIBITED.



CONSOLIDATED STERILIZER SYSTEMS

Consolidated Sterilizers Designed to Transform Your Laboratory

Models	
SR-24C (24' x 36" x 36")	
SR-24D (24' x 36" x 48")	
SR-24E (24' x 36" x 60")	
SR-24F (24' x 36" x 72")	
SR-26B (26' x 26" x 48")	
SR-28B (28' x 28" x 48")	

Medium Lab Series Steam Sterilizers General Specifications

General Specification

Steam Sterilizer, Radial-Arm Door(s), Hinged, Single Chamber, Double Wall

Consolidated Medium Lab Series Sterilizers are designed to sterilize at temperatures between 212° F and 275° F (100° C and 135° C) through the use of steam. Choose from a variety of sizes and programmable control options for pre-vacuum or gravity operation. Consolidated Sterilizers offer a range of performance options to meet the most demanding applications in clinical, animal and life science, biotechnology, pharmaceutical, and commercial/industrial applications.

Features and Benefits

Simplified Maintenance, Low Cost of Ownership.

All Consolidated sterilizers are manufactured in the USA and built from commonly available parts to allow quick and cost effective field-level service and maintenance.

Serviceability.

Easy access to replaceable components, local component availability and common electrical and plumbing parts permit qualified facility or area service companies to maintain the sterilizer.

Control Flexibility.

A choice of programmable controllers allows a broad range of performance functions, complete with alarm, monitoring and communications required for internal or third-party compliance.

Performance Cycles—Basic to Advanced.

The fully-jacketed sterilizer design permits vacuum and pressure control when configured for pre-vacuum, post-vacuum, and more sophisticated functions such as air-over-pressure. Consolidated sterilizers are ideal for sterilizing wrapped and unwrapped goods, liquids, waste, and other applications.

Green and Environmentally Friendly.


Unique, new technologies reduce water and energy consumption without compromising performance.

Cloud-Enabled

Consolidated sterilizers connect to the internet and are pre-configured for cloud-based monitoring, alerting and data collection.

Table of Contents

- Model Sizes and Weights.....2
- Sterilizer Construction.....2
- Sterilization Cycles.....6
- Options & Accessories.....8
- Installation.....9
- Footprint Drawings.....10
- Utility Information.....12

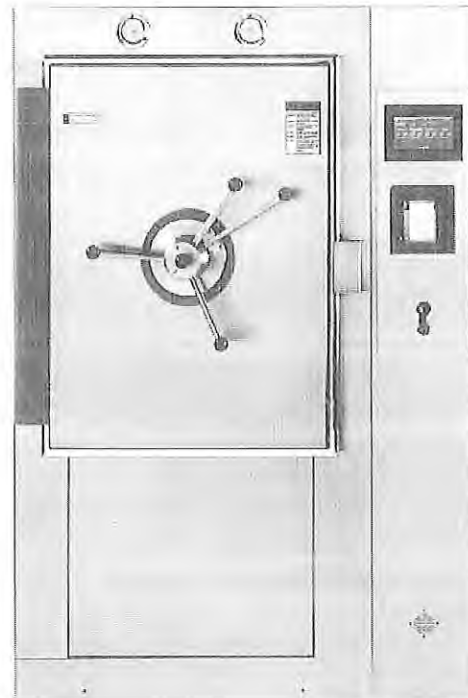

Consolidated Medium Lab Series Sterilizers are available in single door, and pass-thru models. A versatile control system offers a range of performance options to meet the most demanding applications in life science, biotechnology, pharmaceutical, and commercial/industrial applications. Model SR-24D-X1 shown with X1™ control system.




MODEL SIZES & WEIGHT

Summary Selection Chart

Consolidated Medium Lab Series sterilizers are based on five chamber sizes, both single door and pass-thru models. All doors are right-hinge, standard. Optional left-hinge doors must be specified when ordering.


Model	Chamber Dimensions (W x H x D)	Volume (cu. ft./liters)	Ship Weight (lbs/kg)	Ship Dimensions (W x H x D)
-------	-----------------------------------	----------------------------	-------------------------	--------------------------------

Single Chamber Models



SR-24C	24" x 36" x 36" 61 x 91.4 x 91.4 cm	18 cu. ft. 510 liters	2,700 lbs 1,228 kg	46" x 78" x 65" 116.8 x 198.1 x 165.1 cm
SR-24D	24" x 36" x 48" 61 x 91.4 x 122 cm	24 cu. ft. 680 liters	3,150 lbs 1,432 kg	46" x 78" x 78" 116.8 x 198.1 x 198.1 cm
SR-24E	24" x 36" x 60" 61 x 91.4 x 152.4 cm	30 cu. ft. 850 liters	3,600 lbs 1,637 kg	46" x 78" x 89" 116.8 x 198.1 x 226.1 cm
SR-24F	24" x 36" x 72" 61 x 91.4 x 183 cm	36 cu. ft. 1,019 liters	4,300 lbs 1,955 kg	46" x 78" x 98" 116.8 x 198.1 x 248.9 cm
SR-26B	26" x 26" x 49" 66 x 66 x 124.5 cm	19.2 cu. ft. 544 liters	2,700 lbs 1,227 kg	46" x 77" x 79" 116.8 x 195.6 x 201 cm
SR-28B	28" x 28" x 48" 71 x 71 x 122 cm	21.8 cu. ft. 617 liters	2,980 lbs 1,355 kg	48" x 78" x 78" 122 x 198.1 x 198.1 cm

Single Chamber, Pass-thru Models



PT-SR-24C	24" x 36" x 36" 61 x 91.4 x 91.4 cm	18 cu. ft. 510 liters	3,150 lbs 1,432 kg	46" x 78" x 74" 116.8 x 198.1 x 188 cm
PT-SR-24D	24" x 36" x 48" 61 x 91.4 x 122 cm	24 cu. ft. 680 liters	3,600 lbs 1,637 kg	48" x 78" x 87" 122 x 198.1 x 221 cm
PT-SR-24E	24" x 36" x 60" 61 x 91.4 x 152.4 cm	30 cu. ft. 850 liters	4,050 lbs 1,841 kg	48" x 81" x 98" 121.9 x 205.7 x 248.9 cm
PT-SR-24F	24" x 36" x 72" 61 x 91.4 x 183 cm	36 cu. ft. 1,019 liters	4,750 lbs 2,160 kg	48" x 81" x 104" 122 x 205.7 x 264.2 cm
PT-SR-26B	26" x 26" x 49" 66 x 66 x 124.5 cm	19.2 cu. ft. 544 liters	3,050 lbs 1,386 kg	46" x 77" x 79" 116.8 x 195.6 x 201 cm
PT-SR-28B	28" x 28" x 48" 71 x 71 x 122 cm	21.8 cu. ft. 617 liters	3,350 lbs 1,523 kg	48" x 78" x 87" 122 x 198.1 x 221 cm

High Performance Sterilization

Consolidated sterilizers are used in a wide range of applications including clinical, animal and life science, biotechnology, pharmaceutical, and commercial/industrial markets. Consolidated sterilizers are suitable for conventional or pre-vacuum sterilization for quality control, safety and regulatory compliance. In addition, all units can be customized to suit any unique requirements and applications of a particular facility.

Consolidated uses only commonly-available, open-source parts in all phases of sterilizer design and construction, thereby permitting quick, economical and locally-managed service throughout the life of the product. With maximum uptime engineered into the product, Consolidated sterilizers offer a superior return on investment as demonstrated through thousands of installations worldwide.

STERILIZER CONSTRUCTION

Sterilizer Chamber

Consolidated steam sterilizer vessels are manufactured with an inner chamber and a full outer jacket. The inner chambers are available in either Type 316L stainless steel or nickel-clad steel construction. Jacket construction is available in carbon steel, Type 304L stainless steel or Type 316L stainless steel. Material selection is directly related to the chemical properties of available water supply and intended application. All vessels with Type 316L stainless steel inner chambers are polished to a high luster finish and passivated. Pressure vessels are welded in compliance with ASME Section VIII, Division I.

Chamber Door and Gasket System

Consolidated's sterilizer doors are designed with redundant, independent mechanical and software features to ensure maximum safety. Door design specifications meet all ASME code requirements.

- Multiple door arms assure that, in the event of a failure of any one arm, the door will continue to support the load within performance specifications.
- Door engagement is clearly visible to confirm closure.
- An electrical door switch ensures that the door is fully closed and locked prior to the start of the cycle. If the signal is lost during a sterilizing cycle, the cycle is automatically aborted.
- The door pressure clutch assembly is activated by chamber pressure to lock the door. Chamber pressure forces a membrane against the clutch plate, engaging the lock to permit tightening, but not loosening of the door.
- As the handle is turned to the closed position, the latching arms extend out into the door end-frame. Full rotation of the door handle presses the door against the chamber sealing surface thereby compressing the seal, and activating the electrical door limit switch.
- Consolidated hinged door autoclaves use solid silicone gaskets that do not require high pressure air, steam or vacuum to operate. Instead, the act of closing the door compresses the silicone gasket to create a secure and reliable seal. In the event that the gasket fails, the door can still be easily opened and the gasket quickly replaced.
- Pass-thru (double-door) sterilizers may be ordered with optional door interlocks. This electro-mechanical lock on each door minimizes the chance of cross-contamination between contained and uncontained areas by preventing both doors from being opened simultaneously. Additionally, this feature prevents the uncontained side door from opening under non-sterile conditions.

Components

- Piping, fittings, and valves are available in stainless steel or brass/bronze. All parts and components subject to repair are publicly available (i.e. non-proprietary) from open market sources, including controls, valves and fittings.
- Safety relief valves and drains are integral to the plumbing configuration.
- Baffled steam inlets minimize direct condensate on the load, reduce load wetting, and help assure proper steam uniformity within the chamber.
- Cabinet insulation retains heat and minimizes heat loss (see Table 10) to the room. The sterilizer jacket and all steam service piping include a minimum 1" fiberglass-based insulation.
- An integral wastewater cooling function reduces discharge temperature to the drain to less than 140° F (60° C).

- On units equipped with steam generators, a manual reset pressure switch is included to back up the safety relief valve by automatically shutting down the steam generator if an overpressure condition exists.
- Easy-to-read pressure gauges ensure simple and safe operation.
- Other components required for the intended application may include a steam generator, vacuum pump, water ejector, etc. depending on the options chosen.

Control and Monitoring System

Consolidated offers a state-of-the-art control system built from industry standard, open source components for international availability of parts and service. Consolidated's X1™ controllers offer proven reliability, based on an industrial PLC platform programmed specifically for Consolidated's sterilizers, complete with modern user interface and an intuitive touchscreen display (see chart on page 4).

- Permits industry standard and custom sterilizer cycles.
- Simplifies operation with intuitive operator interfaces and options allow the ability to add favorite shortcuts for frequently used cycles and ability to prevent users for modifying sterilization parameters on individual cycles.
- Assures quality control and process integrity.
- Features sterilizer cycle quality reporting and printed documentation.
- Audible and visual alarms warn of cycle or other deviations.

Cloud-Based Monitoring and Data Collection

All Consolidated sterilizers have the ability to connect to the internet (via Ethernet or Wi-Fi) to allow remote monitoring, alerting and data collecting. All data is secured using HTTPS/TLS encryption and protected using 2-factor authentication. This system has the following capabilities:

- View the real-time status of the autoclave from any computer, smart phone or tablet using a standard web browser.
- Subscribe to and receive SMS/text and email alerts regarding cycle completion, cycle abort, alarm conditions, PM reminders and usage tips.
- View and download historical cycle data showing User ID, cycle name, cycle time, cycle completion status and all errors or alarms, as applicable.

Calibration

All temperature and pressure sensors on the sterilizer can be calibrated using an intuitive three-point calibration method.

Printer

An impact printer can be integrated into the main control panel. Printout includes all important information regarding the sterilization cycle recorded at user-defined intervals. Information includes: operator identification, cycle type, cycle parameters, cycle phase, time, chamber pressure and temperature, alarms or messages and cycle completion status.

Alarms

Detailed performance and function alarms are included with the X1™ controller, as well an alarm history report visible on the touchscreen. Standard safety alarms are included in all Consolidated sterilizers.

Cycle Safeguards

The following cycle safeguards help assure safe operation.

- No cycle can start unless the door is properly closed and locked.
- Control inputs automatically reject incorrect cycle parameters.
- Chamber gauges are installed on the operating end of the sterilizer to display pressure in psig and vacuum in inches-Hg.
- Exhaust is automatically condensed and cooled to a safe drainage temperature.
- Multi-rate liquid exhaust allows users to select an exhaust rate above and below an adjustable temperature set-point. This prevents boil-over of liquids and reduces total cycle time.

Steam Sources

Consolidated sterilizers can operate on house steam or steam produced by integral or remote steam generators. Incoming water quality is always a primary consideration in selection of a steam generator (see Table 9).

Selection of the steam source is based on facility steam availability and other factors associated with sterilizer use and throughput.

House Steam

In most situations standard house steam, when available, is adequate. An inlet steam filter may be required to clean the steam prior to injection into the sterilizer plumbing system.

Electric Steam Generator

When house steam is not available, an electric boiler must serve as the steam source. Higher wattage generators produce a higher rate of steam to the chamber. Standard voltages available are 208, 240, 380, 480. Three-phase or single-phase voltage connections are available.

- Integrated Boiler.

Consolidated can provide an integral (fits under the sterilizer chamber) steam generator up to 45 kW.

A standard steam boiler, constructed of carbon steel, is utilized on units fed with tap, softened or RO water. (See Table 9 for water quality requirements).

A clean steam boiler, constructed of type 316L stainless steel, is required when the water quality feed is >1 MΩ·cm. This option typically requires that the sterilizer be constructed with a stainless-steel chamber, jacket, and plumbing.

- Remote Boiler.

Steam generators >45 kW are typically too large to fit beneath the sterilizer chamber and must be remote mounted.

Electric/Steam Combination

Sterilizers can be configured to accommodate both house steam and an integral electric generator. This feature allows for easy switching between either steam sources.

Steam-to-Steam Generator

A steam-to-steam generator delivers clean steam to the sterilizer. Contact Consolidated for details and ordering information.

Consolidated Sterilizer Systems – The X1™ Control System

Consolidated's X1™ controllers offer proven reliability, based on an industrial PLC platform programmed specifically for Consolidated's sterilizers. The X1 control system has an intuitive user interface with modern touchscreen display and can be equipped with up to 50 programmable cycles. The entire system is built from industry-standard, open-source components for international availability of parts and service.

Operator Interface	
Display	7" Widescreen Color
Resolution	WVGA 800 x 400
Mounting Options	Front and Remote Panel

Industry Standard and Advanced Sterilizer Cycles* - Up to 50 Programmable Cycles	
• Gravity	• Vacuum Leak Test*
• Liquids	• Air-Over-Pressure*
• Custom Cycles*	• Rapid Cool*
• ATF Bioreactor*	• Steam-Air Mix*
• Pre-Vacuum*	• Fo with Controlling Load Probe*
• Post-Vacuum Drying*	• Continuous (Product Lifecycle Testing)*
• Low Temperature (isothermal) *	• Bowie-Dick (Air Removal Test)*

Sterilizer Control	
Configurable Cycle Parameters	Standard
Improper Parameter Rejection	Standard
Three Point Calibration of Sensors	Standard
Automatic Condensate Exhaust Management for all Cycles	Standard
Memory Backup of Configuration	Standard
Ability to Favorite Cycles	Optional

Green Features	
Energy Saver EcoCalendar for Scheduled On/Off Steam Supply	Standard
Auto Idle Shut-Off	Standard

Security and Process Integrity	
2 Usernames	Standard
Multi-layered Password Security for Manager and Service	Standard
Ability for Manager to Lock Cycle Configuration and Parameters	Optional
User Traceability Password Protection	Optional
Up to 50 Usernames and Passwords	Optional

Documented Cycle Data Information	
User Defined Cycle Name	Standard
Start Time and Date	Standard
Cycle Type	Standard
Chamber Temperature/Pressures	Standard
Cycle Summary	Standard
Username	Standard
Cycle Set Points and Parameters	Standard
Alarms	Standard

Audible Alarms (Also Displayed on Touchscreen)	
Cycle Completed, Recycle, Over Temperature, Over Pressure, Time Limit, Chamber Drain, Jacket/Chamber Flow Failure	Standard
Alarm History Report on HMI	Standard

Connectivity and Record Keeping	
Cloud-Based Monitoring & Data Collection	Standard
SteriNET™ Connex (Remote Troubleshooting)	Optional
Dry Contacts for Door Open, Cycle Complete, Alarm Condition, or Cycle in Progress	Optional
Printer	Optional

* Optional cycles

EcoCalendar™

The X1 controls are equipped with a calendar-based automatic start-up and shut-down feature known as EcoCalendar. This feature helps minimize utility consumption and HVAC load through a software controlled, automatic steam shut-off program.

Auto Idle Shut-Off

Like the EcoCalendar, this feature helps save energy by shutting the autoclave off when not in use. It functions similarly to a "sleep-mode" for your home computer. Simply set the desired idle time and the autoclave will enter Sleep Mode after the set idle time has elapsed.

Generator Blowdown

In facilities where water quality is poor, a generator blowdown function is required to flush impurities from the system and prevent collection of contaminants on the heating elements. The blowdown function can be initiated manually or ordered as an automatic blowdown function if desired.

Air Removal

Depending on the application and required cycle, air removal may be achieved by gravity displacement or mechanical assistance through vacuum for pre- and post-cycle use as required.

- For gravity air removal, the control system automatically opens and closes valves on demand.
- For pre-cycle vacuum, Consolidated offers a choice of a water-ejector vacuum system, or a water-minimizing liquid ring pump.
- For post-cycle vacuum where drying assistance is desired, the sterilizer can use a water-ejector vacuum system or a water-minimizing liquid ring pump.
- Following completion of the post-vacuum function and throughout return to ambient pressure equilibrium, the returning air is filtered through a 0.3 micron bacteria-retentive HEPA filter.

Shelving

Shelves, carts and other accessories are available to suit specific applications. Shelves and racks are constructed of electro-polished Type 316L stainless steel. Interior shelving options include:

- Standard: One (1) stationary full-length wire-grid bottom shelf and one (1) upper stationary shelf suspended in the middle of the chamber on shelf brackets.
- Option 1: One (1) stationary full-length wire-grid bottom shelf and one (1) upper extendable shelf suspended in the middle of the chamber on shelf brackets.
- Option 2: One (1) stationary full-length wire-grid bottom shelf and two (2) upper extendable shelves suspended on two evenly spaced supports.

Sterilizer Mounting

Consolidated sterilizers are available for installation as floor-standing cabinet-enclosed units with a stainless-steel superstructure to conceal plumbing and wiring. These sterilizers are also available for installation as recessed in one or two walls. Hook-ups for utility connections can be located anywhere on the unit as required, however house connections must be within 5 feet of the unit unless otherwise specified prior to installation.

For Biological Safety Level 3 installations a Bioseal® can be installed to maintain the contamination integrity of the clean side. Utilities can be mounted at the non-contained side of the installation and in the front, rear or designated side of the cabinet.

Water Quality Compatibility (Stainless Steel vs. Non-Stainless Selection)

Materials that contact the water supply to the sterilizer, including the steam generator, water-cooled devices, water-actuated accessories, valves and piping must be compatible with the purity of the water.

- If deionized or distilled water or water with a purity greater than 1 MΩ•cm is supplied, then all such points of contact must be of stainless steel construction.
- If softened water, water purified by reverse osmosis or tap water with purity of less than 0.2 MΩ•cm is supplied, then such points of contact must be of carbon steel, bronze or brass construction, as appropriate.

Compliance and Certifications

Depending on desired application, Consolidated sterilizers can be certified for compliance to the following standards for performance and safety.

- ASME (American Society of Mechanical Engineers): Section VIII, Division I (Unfired Pressure Vessel) code.
- ASME: Section I Code (Miniature Boilers).
- CRN (Canadian Registration Number): requirements for pressure vessels.
- IEC (International Electrotechnical Commission):
 - EN 61010-1:96—Safety requirements for electrical equipment for measurement, control, and laboratory use.
 - EN 61010-2-041:96—Specific requirements for steam autoclaves.
- UL and cUL (Underwriters Laboratory): Standard 61010-1 and 61010-2.
- US NEC (National Electrical Code) and National Plumbing Code; NFPA-70.
- EN ISO 111345-R-8/93—AAMI (Association for the Advancement of Medical Instrumentation) Industry Standard for Moist Heat Sterilization.
- 21 CFR Part 11 (US Code of Federal Regulations, Section 21—Food and Drugs; Electronic Records; Electronic Signatures).
- ANSI/AAMI ST-8: Hospital Steam Sterilizers.

Sterilization Cycles

Consolidated sterilizers can be easily configured for numerous cycles and functions. Each cycle is customizable to meet user specific requirements. All cycle parameters are easily viewed prior to and during the cycle run. The following cycles are pre-configured and installed on all sterilizers:

Gravity

The gravity cycle uses gravity to displace the air in the chamber with pressurized steam. This cycle is used mainly for unwrapped goods. The operator may select a sterilization temperature anywhere between 212° F and 275° F (100° C and 135° C), as well as sterilization time and dry time (see Figure 1).

Liquids

The liquid cycle prevents boil-over when vented liquids are sterilized. The controller is factory-configured to automatically release steam pressure at an adjustable exhaust rate. The operator may select a sterilization temperature anywhere between 212° F and 275° F (100° C and 135° C), as well as sterilization time (see Figure 2).

Additional Sterilization Cycles (available upon request)

Gravity with Post-Vacuum Drying

Available on gravity and pre-vacuum units. This cycle draws a vacuum following sterilization and significantly decreases drying time. Post-vacuum is usually used for wrapped goods, fibers, rubber, bedding, glassware and similar loads. The operator may select a sterilization temperature anywhere between 212° F and 275° F (100° C and 135° C), as well as sterilization time and dry time (see Figure 4).

Liquids with Load Probe

Available on gravity and pre-vacuum units. This cycle uses a temperature probe placed within the liquid load to detect, display and print temperature. Applications include sterilization of temperature-sensitive liquids or large volume liquid sterilization (i.e. >2 liter flasks).

Pre-Vacuum

Available only on pre-vacuum units. This cycle performs a series of steam pulses and vacuum draws prior to sterilization to assure that air has been removed from the load. This also permits the ability to vacuum dry. The number of pulses, pulse steam pressure, vacuum pulse pressure, sterilization time and temperature, and dry time are customizable for each cycle (see Figure 3).

Bowie-Dick (Air Removal Test)

Available on pre-vacuum units. This air-removal test cycle validates the vacuum function using ad hoc test packs as per requirements listed in AAMI ST-8.

Vacuum Leak Test

Available on pre-vacuum units. This cycle provides easy verification of vacuum depth, vacuum seal and chamber piping integrity. Detects leaks greater than 1 mmHg (1 Torr) per minute.

Effluent Decontamination

Available on gravity and pre-vacuum units. Retains liquid effluent, if any, within the chamber for the duration of the sterilization cycle. Aerosol effluent passes through a 0.2 micron hydrophobic HEPA filter with >99.999% efficiency; the filter is located within the chamber and is sterilized *in situ* to eliminate the need for disposal after each cycle. The filter is easily replaced by the user when required without special tools or service personnel.

Air-Over-Pressure

Available on gravity and pre-vacuum units. This cycle uses compressed air to maintain chamber pressure at the sterilization pressure until the liquid has cooled to a user adjustable temperature. This is useful for small volumes of liquid susceptible to boil-over (see Figure 5).

Low Temperature

Available on gravity and pre-vacuum units. Typically used for temperature-sensitive goods, this function creates a zero-pressure, temperature only cycle between 190° F and 212° F (88° C and 100° C). Often referred to as an isothermal or inspissation cycle.

Rapid Cooling

Available on gravity and pre-vacuum units. Useful for rapidly cooling liquid media via an interior water spray mechanism or jacket quench, post-sterilization.

F₀ Cycle

Available on gravity and pre-vacuum units. Useful for heat-sensitive liquid media. Sterilization begins when temperature reaches 212°F and is completed when the F₀ set-point is reached. F₀ is adjustable.

Temperature/Pressure Ramping

Available on gravity and pre-vacuum units. Allows the user to specify a) the amount of time it takes for the load to rise to sterilization temperature/pressure and b) the amount of time it takes to exhaust the sterilizer chamber post-cycle. Ideal for loads that are sensitive to rapid pressure changes.

Continuous

Any sterilization cycle can be programmed to be continuously repeated (number of times is adjustable) without any input from the operator. Used for product lifecycle testing.

Steam-Air Mix

Useful for liquid-filled syringes or other sealed containers. Sterilization occurs at an elevated pressure relative to temperature. Extra pressure is achieved using a house air source.


ATF Bioreactor Cycle

The ATF bioreactor cycle is designed to permit the sterilization of hollow fiber filters while housed in bioreactors. ATF (Alternating Tangential Flow) is a technology used in the perfusion culture of mammalian cells, proteins and antibodies. This cycle incorporates a series of temperature ramps and hold times to prevent damage to the fiber filter.

Sterilizer Cycle Selection


Gravity. (Figure 1)

Steam flows through the sterilizer, temperature and pressure ramps slightly to a continuous flow purge. The controller closes the exhaust valve and interior temperature and pressure ramp up to desired setpoint. The program maintains dwell until desired time is reached, when pressure is released. The interior is restored to ambient pressure although contents remain relatively hot.

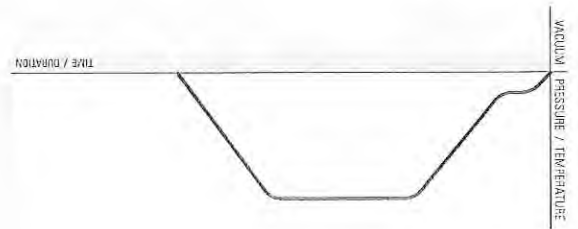


Liquid. (Figure 2)

Steam flows through the sterilizer, temperature and pressure ramps slightly to a continuous flow purge. The controller closes the exhaust valve and interior temperature and pressure ramp up to desired setpoint. The program maintains dwell until desired time is reached. Pressure is gradually released to allow dissolved gases to reach equilibrium to prevent boil-over.

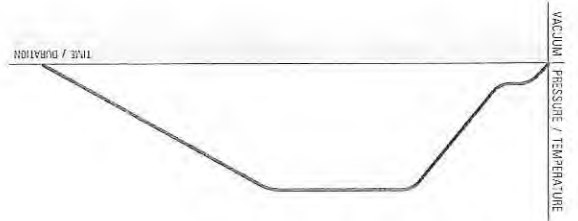


Pre-Vacuum with Post-Vacuum Drying. (Figure 3)

Steam flows through the sterilizer, temperature and pressure ramps slightly to a continuous flow purge. The controller closes the exhaust valve and interior temperature and pressure ramp to an intermediate setpoint without dwell. A vacuum system draws the interior atmosphere to negative pressure to remove latent air from concealed pockets within the load. The process is repeated per program and protocol. Following the final pre-vacuum pulse, the sterilizer ramps to desired setpoint. The program maintains dwell until desired time is reached, when pressure is released. If a post-vacuum program is used, a vacuum system draws the interior atmosphere through ambient to negative pressure, accelerating drying time as programmed, after which the vacuum is released and the load is restored to ambient pressure. If a post-vacuum program is not used, the load is restored to ambient pressure.

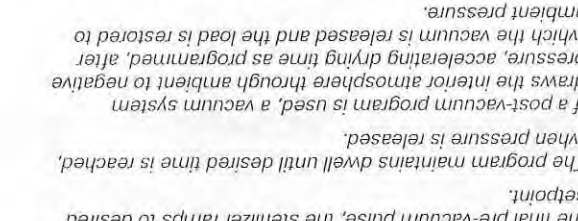


Pre-Vacuum with Post-Vacuum Drying. (Figure 3)

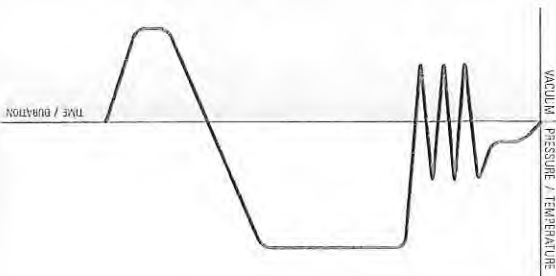

Gravity with Post-Vacuum Drying. (Figure 4)


Steam flows through the sterilizer, temperature and pressure ramps slightly to a continuous flow purge. The controller closes the exhaust valve and interior temperature and pressure ramp up to desired setpoint. The program maintains dwell until desired time is reached, when pressure is released. A vacuum system draws the interior atmosphere through ambient to negative pressure, accelerating drying time as programmed. Once completed the vacuum is released and the load is restored to ambient pressure.

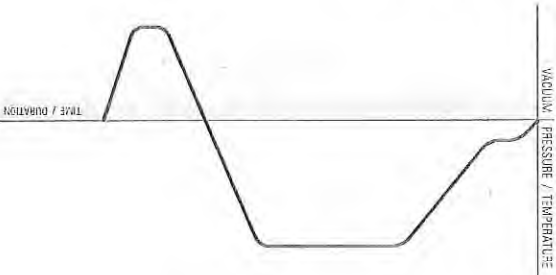

Liquid, Air-Over-Pressure. (Figure 5)

Usually used with smaller amounts of media to prevent liquid loss.

The air-over-pressure function operates identical to the liquid cycle except that pressurized air is injected to cool the load while maintaining pressure to displace steam. After sterilization, air is injected, pressure is maintained, this prevents boil-over and minimizes evaporation. Air pressure is then released and the load is restored to ambient pressure.

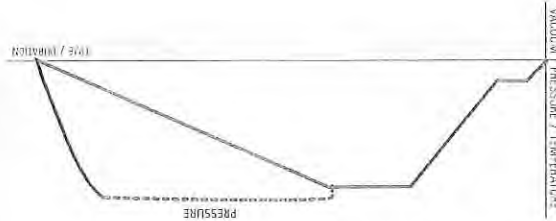

Options & Accessories

Consolidated offers a range of options and accessories to optimize and customize your sterilizer, to meet requirements for internal or third-party compliance, and to improve workflow. Some options are factory installed and must be specified when ordering. Contact Consolidated for detailed information on any of the following:

WaterEco® Water Saving Systems

The Consolidated WaterEco® Water Saving Systems reduce water consumption to the autoclave by up to 99%. Factory or field installed. Available on gravity and pre-vacuum units in the following configurations:

- **WaterEco® Basic:** Reduces cooling water by up to 90% without the use of electricity. This system functions by collecting autoclave drainage into a cooling reservoir. This effluent is cooled using a combination of air, previously cooled effluent and a minimal amount of cold water.
- **WaterEco® Plus:** Reduces water consumption by up to 99% through a stainless steel heat exchanger that utilizes facility chilled water supply. This system virtually eliminates once-through cooling water.
- **WaterEco® Vac Plus:** This full recovery system reduces water consumption by the vacuum system by up to 99%. Designed to integrate with pre-vacuum autoclaves when facility chilled water is readily available. This system is the best solution to minimize water consumption.

Water Purification System

High-purity water purification systems are available for facilities that do not meet the minimum water purity requirements (see Table 9) or that require clean steam. Option 1: A reverse osmosis (RO) water filtration system designed to pre-treat autoclave feed-water can be supplied (Model WPS-1200-RO). Option 2: If deionized water is required for clean steam generation, an RO/DI system that incorporates extra filtration to produce Type II deionized water ($>1 \text{ M}\Omega$ resistivity) can be supplied (Model WPS-1200-DI).

Steam Generator

For installations where house steam is not available, a variety of integral or remote mounted steam generators is available. Consolidated will assist with selection according to site preparation requirements. Generators are available in electric, or steam-powered configurations. Integral generators are factory installed and must be specified when ordering.

Automatic Generator Blowdown

Recommended to remove accumulated impurities from the steam generator when used with low quality incoming water. Factory installed. Specify when ordering.

Steam Inlet Filter

Recommended to clean dirty steam (i.e. remove particulates) from facility steam sources. Specify when ordering.

Nickel-Clad Chamber

Recommended chamber material for sterilizing high-concentration salt solutions or if the feed-water or tap-water for steam generation has high chloride content. Specify when ordering.



SteriNET® Remote Monitoring and Troubleshooting

SteriNET® Connex permits Consolidated engineers to provide quick, accurate and economical offsite diagnosis of operation problems through a standard phone line or Ethernet connection. This option is ideal for facilities located in remote areas where service assistance is hours or days away. This option includes one year of free, remote-transmitted software upgrades from the Consolidated technical support center.

RS-232 Port

Connects the control system to data logging/monitoring equipment. Factory installed. Specify when ordering.

Steril-Q™ Validation Services & Documentation

Protocols and templates are available for Factory Acceptance Testing (FAT), Installation Qualification (IQ), Operation Qualification (OQ), Performance Qualification (PQ) and steam Quality (SQ) testing. Specify when ordering.

Load Probe

Includes a temperature probe with lead wire permitting placement in the load to be sterilized such as liquid, red-bag or other. Sterilization cycle time is based on load temperature instead of chamber temperature. Factory installed. Specify when ordering.

Multi-Probe Sealing Gland

Multi-port gland permits safe installation of thermocouples or other probes inside the chamber. Factory installed. Specify desired quantity and location when ordering.

Automatic Jacket Blowdown

Recommended for liquid cycles. This option is used to exhaust steam in the chamber as well as the jacket to prevent liquid loads from boiling over. Factory installed. Specify when ordering.

Seismic Anchorage Details

May be required to meet building codes in seismically active areas. Contact your facility manager to determine if required. If ordered, Consolidated will provide anchor attachment points and suggested seismic anchorage details. Specify when ordering.

Sump Pump

Required when gravity drain is not available. Provides positive pump to remove condensate effluent to hard-plumbed drain. Specify when ordering.

Form C Dry Contacts

Offers direct connection to building monitoring system (120 VAC output). Specify desired outputs when ordering: door open/close, power on/off or sterilize alarm conditions. Specify when ordering.

Chamber Finish

- High polish (mirror finish), less than 10Ra.
- Passivation and Electropolish.

Stainless Steel Piping

- Upgrade from brass/bronze piping & components to type 316 stainless steel for all product wetted surfaces.

Flood Switch

In the event of excessive liquid in the chamber or jacket, an alarm will sound and a message will be displayed warning the user about the flood condition. Factory installed. Specify when ordering.



Uninterruptible Power Supply (UPS)

Allows the control system to remain on in the event of a brief power loss or brownout. Specify when ordering.

Loading Cart & Transfer Carriage

A loading cart, mounted on rollers, with two stainless steel shelves and a wheeled transfer carriage. The transfer carriage mates to interior guide rails to ease loading and unloading of sterilization loads up to 500 lbs evenly distributed.



Pass-Thru (Double-Door) Options

Pass-thru Door Interlock System

For pass-thru models only. Prevents opening of the sterilizer door on the non-contained side until completion of a sterilization cycle. Also prevents both doors from being opened simultaneously. This system is programmed to accommodate the desired direction of product flow and is equipped with a secondary touchscreen controller located on the non-contained side. Typically a requirement for BSL-3 labs. Factory installed. Specify when ordering.

Dual Controls

For pass-thru models only. Provides full touchscreen controls mounted on each end of the unit for operation from within or outside the containment area. Printer, if included, located outside containment area only unless otherwise specified. Specify when ordering.

Remote-Start Touch Screen

For pass-thru models only. Provides touchscreen controls on the non-contained side capable of starting/stopping the cycle. Specify when ordering.

Bioseal® Biological Sealing Flange

The Bioseal® biological sealing flange, required for Biological Safety Level-3 (BSL-3) applications, employs a stainless steel barrier flange welded to the periphery of the sterilizer and another stainless steel barrier is attached to the wall opening through which the sterilizer is installed. This arrangement is used to prevent the passage of airborne microorganisms from the contained side of the sterilizer to the uncontained side. A single piece closed-cell silicone gasket completes the seal between the building and the sterilizer thereby ensuring seal integrity is not compromised during normal expansion and contraction of the building. Specify when ordering.

Air Differential Seal

An Air Differential Seal is required for applications that require a negative or positive air pressure differential between two rooms adjoined with an autoclave. The seal prevents the bulk passage of air between areas maintained at a pressure differential. A stainless steel barrier flange is welded to the periphery of the sterilizer and closed-cell gasket secures the welded seal to the wall and permits normal expansion and contraction of the building. Specify when ordering.

Vermin Seal

A vermin seal employs a metal barrier to impede rodents from passing through the space between a recessed-mounted autoclave and the wall opening. This is useful if a recessed autoclave is located in the same room as live rodents. Specify when ordering.

Effluent Decontamination Control

Exclusively from Consolidated, this effluent decontamination system traps bacteria within the autoclave chamber and sterilizes it prior to release into the drain (Consolidated Patented Process). Any liquid effluent is held in the chamber for the duration of the sterilization cycle. All aerosol effluent passes through a 0.2 micron hydrophobic HEPA filter with >99.999% efficiency. The steam that sterilizes the products in the chamber also sterilizes the bacteria held by the filter. Filters are easily changed after use. Factory installed. Specify when ordering.

Site Preparation and Utilities

General

Utilities of ample capacity required for operation of the sterilizer shall be provided at the place of installation at the facility. Key considerations include electric power availability, steam source, water type and flow capacity, and compressed air (if air-over-pressure cycle is desired). For information on required utilities and locations refer to the sterilizer architectural drawing.

- Drain and ventilation considerations include wastewater and the facility HVAC system.
- Clearances include door and cart allowances, recommended 18–24" for access to plumbing, adequate load-bearing capacity of floor at installation site, and biointegrity.
- Consider the location of sprinklers, smoke detectors, and canopy capture hoods.
- Contact Consolidated or your Consolidated sales representative for planning and selection assistance.

Installation

Consolidated offers a choice of installation options to accommodate the facility schedule. In general, Consolidated can arrange for any of the following installation preferences:

- **Level 1:** Sterilizer start-up and user training.
- **Level 2:** Sterilizer uncrating, setting in place, leveling, final assembly, start-up, and user training.
- **Level 3A:** Sterilizer uncrating, setting in place, leveling, final assembly, final utility connections, start-up, and user training.
- **Level 3B:** Receiving the shipment, sterilizer uncrating, setting in place, leveling, final assembly, start-up, and user training.
- **Level 4 (Turnkey):** Receiving the sterilizer, uncrating, setting in place, leveling, final assembly, final utility connections, start-up, and user training.
- **Installation Supervision:** Consolidated will supervise on-site installation work performed by facility designated labor.

Standard Mounting Configurations

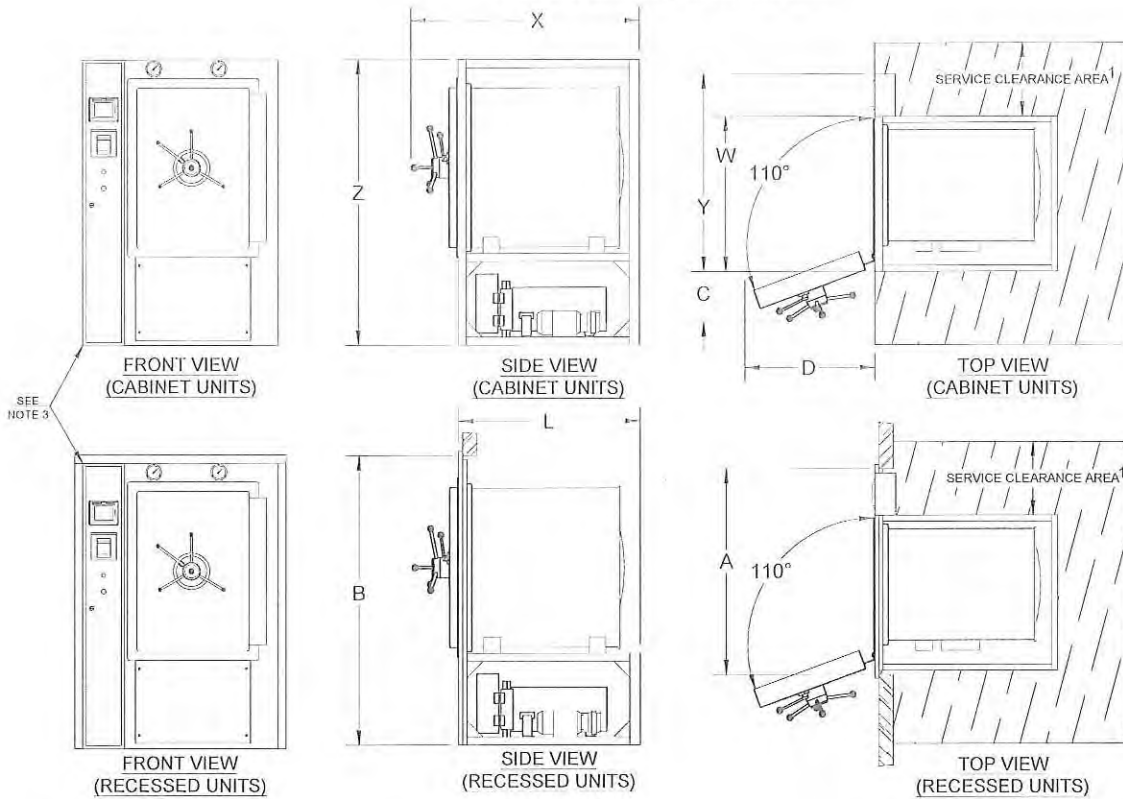


Table 1: Sterilizer Dimensions²

Model	SR-24C	SR-24D	SR-24E ⁶	SR-24F ⁶	SR-26B	SR-28B
Chamber Dimensions (w x h x f-b)	24" x 36" x 36" 61 x 91.4 x 91.4 cm	24" x 36" x 48" 61 x 91.4 x 122 cm	24" x 36" x 60" 61 x 91.4 x 152.4 cm	24" x 36" x 72" 61 x 91.4 x 183 cm	26" x 26" x 49" 66 x 66 x 124.5 cm	28" x 28" x 48" 71 x 71 x 122 cm
Volume	18 cu. ft (510L)	24 cu. ft (680L)	30 cu. ft (850L)	36 cu. ft (1019L)	19.2 cu. ft (544L)	21.8 cu. ft (617L)
Overall Length (X)	56" 142.2 cm	68" 172.7 cm	80" 203.2 cm	92" 233.68 cm	68" 172.7 cm	71" 180.3 cm
Overall Width (Y)	48.375" 122.9 cm	48.375" 122.9 cm	48.375" 122.9 cm	48.375" 122.9 cm	48.375" 122.9 cm	51.375" 130.5 cm
Overall Height (Z) ⁵	71" 180.3 cm	70.25" 178.4 cm	70.25" 178.4 cm	70.25" 178.4 cm	71" 180.3 cm	71" 180.3 cm
Frame Length (L)	45" 114.3 cm	58" 147.3 cm	70" 177.8 cm	82" 208.3 cm	55" 114.3 cm	58" 147.3 cm
Frame Width (W)	38" 96.5 cm	38" 96.5 cm	38" 96.5 cm	38" 96.5 cm	38" 96.5 cm	41" 104.1 cm
Wall Opening Width (A)	50.375" 128 cm	50.375" 128 cm	50.375" 128 cm	50.375" 128 cm	50.375" 128 cm	53.375" 135.6 cm
Wall Opening Height (B)	72" 182.9 cm	71.25" 181 cm	71.25" 181 cm	71.25" 181 cm	72" 182.9 cm	72" 182.9 cm
Door Swing Clearance (C)	20" 50.8 cm	20" 50.8 cm	20" 50.8 cm	20" 50.8 cm	12.75" 32.4 cm	20.5" 52.1 cm
Door Swing (D)	31.5" 80 cm	31.5" 80 cm	31.5" 80 cm	31.5" 80 cm	35.5" 90.2 cm	37.5" 95.3 cm

1) Recommended service clearance is 18-24" both sides and back. If necessary, service clearance can be decreased or adjusted to one side to accommodate facility space constraints.

2) Additional options may require a larger footprint.

3) The control housing is shipped detached from the sterilizer to allow passage through doorways, reducing pre-installation Overall Width (Y) by 10.375". When the sterilizer is installed, the control housing and electrical connections are easily attached.

4) All views contain configuration specific components. These are for illustrative purposes only, actual configuration may vary.

5) After adjustment, leveling feet may add up to 1 inch to the Overall Height (Z).

6) Electric generator is not integral to sterilizer and requires a separate footprint.

This page shows a variant recessed mounting to allow a sterilizer to fit into an existing narrow wall opening

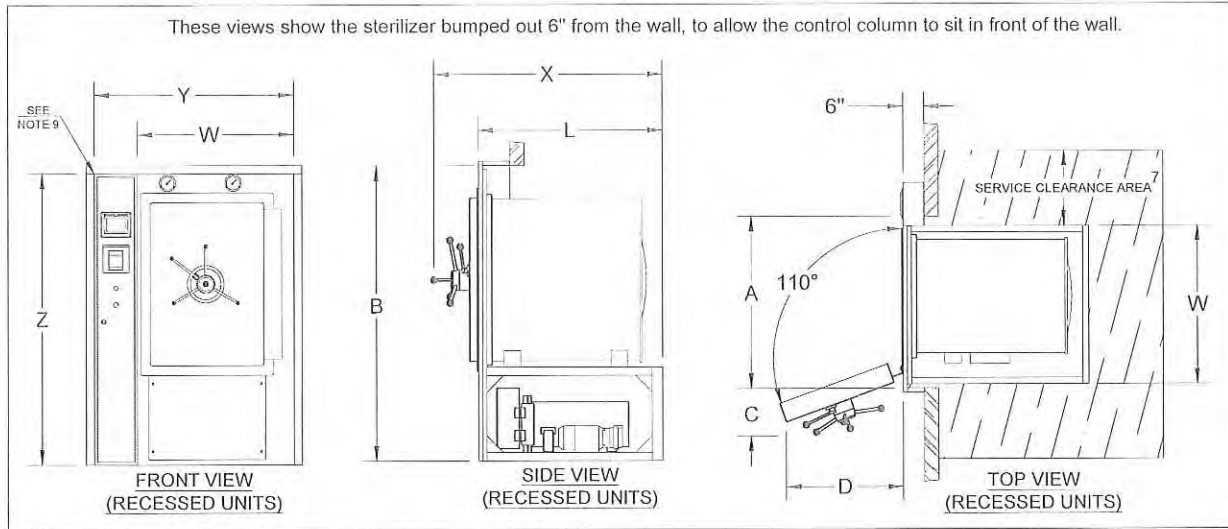


Table 2: Sterilizer Dimensions⁸

Model	SR-24C	SR-24D	SR-24E ¹⁰	SR-24F ¹⁰	SR-26B	SR-28B
Chamber Dimensions (w x h x f-b)	24" x 36" x 36" 61 x 91.4 x 91.4 cm	24" x 36" x 48" 61 x 91.4 x 122 cm	24" x 36" x 60" 61 x 91.4 x 152.4 cm	24" x 36" x 72" 61 x 91.4 x 183 cm	26" x 26" x 49" 66 x 66 x 124.5 cm	28" x 28" x 48" 71 x 71 x 122 cm
Volume	18 cu. ft (510L)	24 cu. ft (680L)	30 cu. ft (850L)	36 cu. ft (1019L)	19.2 cu. ft (544L)	21.8 cu. ft (617L)
Overall Length (X)	56" 142.2 cm	68" 172.7 cm	80" 203.2 cm	92" 233.68 cm	68" 172.7 cm	71" 180.3 cm
Overall Width (Y)	48.375" 122.9 cm	48.375" 122.9 cm	48.375" 122.9 cm	48.375" 122.9 cm	48.375" 122.9 cm	51.375" 130.5 cm
Overall Height (Z)	71" 180.3 cm	70.25" 178.4 cm	70.25" 178.4 cm	70.25" 178.4 cm	71" 180.3 cm	71" 180.3 cm
Frame Length (L)	45" 114.3 cm	58" 147.3 cm	70" 177.8 cm	82" 208.3 cm	55" 114.3 cm	58" 147.3 cm
Frame Width (W)	38" 96.5 cm	38" 96.5 cm	38" 96.5 cm	38" 96.5 cm	38" 96.5 cm	41" 104.1 cm
Wall Opening Width (A)	39" 99.2 cm	39" 99.2 cm	39" 99.2 cm	39" 99.2 cm	39" 99.2 cm	42" 106.8 cm
Wall Opening Height (B)	72" 182.9 cm	71.25" 181 cm	71.25" 181 cm	71.25" 181 cm	72" 182.9 cm	72" 182.9 cm
Door Swing Clearance (C)	20" 50.8 cm	20" 50.8 cm	20" 50.8 cm	20" 50.8 cm	12.75" 32.4 cm	20.5" 52.1 cm
Door Swing (D)	31.5" 80 cm	31.5" 80 cm	31.5" 80 cm	31.5" 80 cm	35.5" 90.2 cm	37.5" 95.3 cm

7) Recommended service clearance is 18-24" both sides and back. If necessary, service clearance can be decreased or adjusted to one side to accommodate facility specific space constraints.

8) Additional options may require a larger footprint.

9) The control housing is shipped detached from the sterilizer to allow passage through doorways, reducing pre-installation Overall Width (Y) by 10.375". When the sterilizer is installed, the control housing and electrical connections are easily attached.

10) Electric generator is not integral to sterilizer and requires a separate footprint.

Typical Utility Requirements

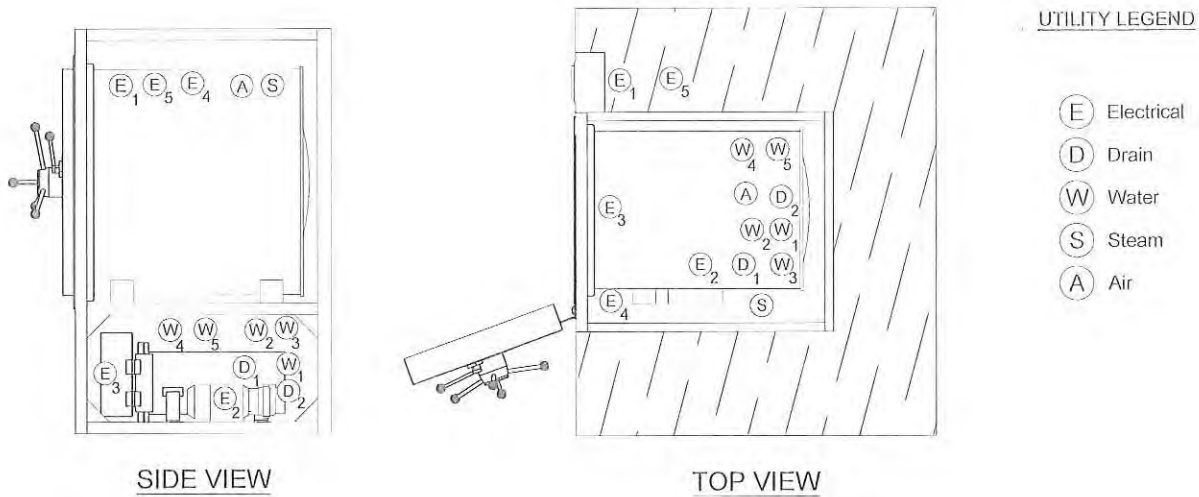


Table 3: General Connections

Name	Symbol	Connection on Sterilizer	MEP Requirements ¹³
Wastewater Cooling	W ₁	1/2" NPT	45 psig dynamic min, 80 psig static max, 3/4"-1" NPT, 12 GPM capacity, with shut off valve and union ¹¹
Controls System	E ₁	NEMA 3-Prong Plug	110V/220V, 20 Amp minimum; non-GFCI outlet
Ethernet Port	E ₅	RJ-45	Standard RJ-45 ethernet cable with internet access
Sterilizer Drain	D ₁	1 1/2" Sweat (NPT on units with WaterEco)	2 1/2" air gap, 3" diameter minimum funnel required, location external to unit footprint recommended
Direct Steam (Optional)	S	1/2" NPT	50-80 psig dynamic, 3/4" NPT, 180 lbs/hr capacity, insulated line with shut-off valve and union
Dry Contacts (Optional)	E ₄	2-Wire Terminal	Signal wires compatible with Form C Dry Contacts
Compressed Air (Optional)	A	1/2" NPT	50 psi dynamic min, 10-35 SCFM, 99% dry & oil free, backflow preventer not provided by CSS

Table 4: Optional Vacuum Systems (maximum one per unit)

Name	Symbol	Connection on Sterilizer	MEP Requirements ¹³
Economy Post-Vac	W ₂	1/2" NPT	45 psig dynamic min, 80 psig static max, 3/4"-1" NPT, 12 GPM capacity, with shut off valve and union ¹¹
Hi-Vac with Water Ejector	W ₂	1/2" NPT	45 psig dynamic min, 80 psig static max, 3/4"-1" NPT, 12 GPM capacity, with shut off valve and union ¹¹
Booster Pump	E ₂	Hard Wire	115V/208-230V, single phase, minimum 20 Amp circuit required
Vacuum Pump - Electrical	E ₂	Hard Wire	208/240/480V, 3-phase, minimum 20 Amp circuit required
Vacuum Pump - Water	W ₂	1/2" NPT	45 psig dynamic min, 80 psig static max, 3/4"-1" NPT, 12 GPM capacity, with shut off valve and union ¹¹

11) W₁ and W₂ cold water connections can be from a single source for a combined 12GPM capacity. Water quality must comply with the General Vacuum Device & Quench specification in Table 9

Table 5: Optional Electric Steam Generator

Name	Symbol	Connection on Sterilizer	MEP Requirements ¹³
Power Supply	E ₃	Hard Wire	Available in 208/240/380/480V, 3-phase, see Table 7 for Amp Draw
Generator Water Feed	W ₃	1/2" NPT	45 psig dynamic min, 80 psig static max, 1/2" NPT, 5 GPM capacity, with shut off valve and union ¹²
Manual Generator Drain	D ₂	1/2" NPT	Route to facility drain

12) Generator feedwater must comply with the Generator Water Feed specification in Table 9.

Table 6: Optional Chilled Water (WaterEco Plus and Vac Plus Units Only)

Name	Symbol	Connection on Sterilizer	MEP Requirements ¹³
Chilled Water Feed	W ₄	1" NPT	20 psi dynamic min, 35°F-50°F max temperature, 10 GPM capacity
Chilled Water Return	W ₅	1" NPT	-5 psi drop on return side, +15°F max rise

13) For a more detailed list of MEP requirements and specifications see "Autoclave Installation and Utility Overview" document.

Table 7: Power and Steam Usage¹⁴

Power and Steam Usage			Electrically Heated				Steam Heated			
Model	Chamber Dimensions (w x h x f-b)	Air Removal Method	Generator Size (KW)	Generator Current (amps) ¹⁵				Peak (lb/hr)	Per Cycle (lb/cycle)	Idle (lb/hr)
				208V	240V	380V	480V			
SR-24C	24" X 36" X 36" 61 X 91.4 X 91.4 cm	Gravity	30	83	72	46	36	180	40	9
		Vacuum	45	125	108	68	54	180	65	9
SR-24D	24" x 36" x 48" 61 x 91.4 x 122 cm	Gravity	30	83	72	46	36	180	45	10
		Vacuum	45	125	108	68	54	180	75	10
SR-24E	24" x 36" x 60" 61 x 91.4 x 152.4 cm	Gravity	60	167	144	91	72	180	50	11
		Vacuum	80-100	222-278	192-240	122-152	96-120	180	105	11
SR-24F	24" x 36" x 72" 61 x 91.4 x 183 cm	Gravity	80	222	198	122	96	180	55	11
		Vacuum	100-120	278-333	240-289	152-182	120-144	180	125	11
SR-26B	26" x 26" x 49" 66 x 66 x 124.5 cm	Gravity	30	83	72	46	36	180	40	9
		Vacuum	45	125	108	68	54	180	70	9
SR-28B	28" x 28" x 48" 71 x 71 x 122 cm	Gravity	30	83	72	46	36	180	40	9
		Vacuum	45	125	108	68	54	180	70	9

14) Assuming 30 Minute sterilizing time at 250°F (121°C) and 5 minute drying time.

15) Nominal current drawn by a 3-phase generator. Local codes and regulations may affect breaker size. Single phase available if required.

Table 8: Water Consumption (Per Chamber)¹⁶

Model	Chamber Dimensions (w x h x f-b)	Air Removal Method	Water Consumption								
			Cold Water					Hot/Treated Water			
			Peak (gpm)	Per Cycle (gal/cycle)	Per Cycle With WaterEco® Basic (gal/cycle)	Idle (gph)	Idle With WaterEco® Basic (gph)	Peak (gpm)	Per Cycle (gal/cycle)	Idle (gph)	
SR-24C	24" X 36" X 36" 61 X 91.4 X 91.4 cm	Gravity	6	30	5	9	1	1	5	1	
		Ejector	6	94	80	9	1	1	5	1	
		Vac Pump	6	50	37	9	1	1	5	1	
SR-24D	24" x 36" x 48" 61 x 91.4 x 122 cm	Gravity	6	40	6	10	1	1	5	1	
		Ejector	6	115	97	10	1	1	5	1	
		Vac Pump	6	65	47	10	1	1	5	1	
SR-24E	24" x 36" x 60" 61 x 91.4 x 152.4 cm	Gravity	6	51	8	10	1	5	6	1	
		Ejector	6	136	113	10	1	5	6	1	
		Vac Pump	6	80	53	10	1	5	6	1	
SR-24F	24" x 36" x 72" 61 x 91.4 x 183 cm	Gravity	6	61	9	11	1	5	7	1	
		Ejector	6	157	130	11	1	5	7	1	
		Vac Pump	6	94	67	11	1	5	7	1	
SR-26B	26" x 26" x 49" 66 x 66 x 124.5 cm	Gravity	6	32	5	9	1	1	5	1	
		Ejector	6	98	84	9	1	1	6	1	
		Vac Pump	6	53	39	9	1	1	6	1	
SR-28B	28" x 28" x 48" 71 x 71 x 122 cm	Gravity	6	37	6	9	1	1	5	1	
		Ejector	6	108	91	9	1	1	5	1	
		Vac Pump	6	60	43	9	1	1	5	1	

16) Assuming 30 minute sterilizing time at 250°F (121°C) and 5 minute drying time.

Table 9: Nominal Water Quality Requirements

Characteristic	Carbon Steel Steam Generators ¹⁷		General Vacuum Device & Quench	
	Recommended Condition	Maximum Condition	Recommended Condition	Maximum Condition
Temperature [°F (°C)]	As Supplied	140 (60)	40-60 (4-16)	70 (21)
Total Hardness (mg/L)	17	85	10-85	171
Alkalinity (mg/L)	50-180	350	50-180	350
Total Dissolved Solids (mg/L)	50-150	250	50-200	500
pH	7.5-8.5	7.5-9.0	6.8-7.5	6.5-9.0
Total Silica (mg/L)	0.1-1.0	2.5	0.1-1.0	2.5
Resistivity (Ω·cm)	2,000-6,000	26,000 ¹⁸	2,000-26,000	500,000

17) Stainless-steel generators require deionized water with resistivity ≥ 1MΩ·cm.

18) If water supplied is greater than 26,000 Ω·cm contact Consolidated for recommendation.

Table 10: Weight & Heat Loss Data

Model	Heat Source	Max. Operating Weight ¹⁹	Peak Heat Loss (BTU/hr at 70°F [21°C])		
			Cabinet		
			To Room	Front of Wall	Back of Wall
SR-24C	Steam	3000 lbs	12550	5000	7500
	Electric	3175 lbs	14800	5800	8950
SR-24D	Steam	3525 lbs	14650	5000	9600
	Electric	3700 lbs	16900	5800	11050
SR-24E	Steam	4075 lbs	16800	5000	11800
	Electric	4075 lbs ²⁰	19050	5800	13250
SR-24F	Steam	4875 lbs	18950	5000	14000
	Electric	4875 lbs ²⁰	21200	5800	15450
SR-26B	Steam	2950 lbs	14390	5000	9400
	Electric	3125 lbs	16140	5700	10500
SR-28B	Steam	3325 lbs	13600	4800	8200
	Electric	3500 lbs	15850	5600	9650

19) Assuming chamber fully loaded with flasks filled 25% with water.

20) Remote Mounted Generator

